



Cleaning Method Validation for Estimation of Dipyrindamole Residue on the Surface of Drug Product Manufacturing Equipment Using Swab Sampling and by High Performance Liquid Chromatographic Technique

İlaç Ürün İmalat Ekipmanının Yüzeyindeki Dipiridamol Kalıntısının Sürüntü Örnekleme ve Yüksek Performanslı Sıvı Kromatografisi Tekniği Kullanılarak Tahmin Edilmesi için Temizleme Metodu Validasyonu

© Sriram VALAVALA¹, © Nareshvarma SEELAM^{1*}, © Subbaiah TONDEPU², © Vivekanandan SUNDARAMURTHY³

¹Koneru Lakshmaiah Education Foundation, Department of Chemistry, Green Fields, Andhra Pradesh, India

²Vignan's Foundation for Science, Technology and Research, Department of Chemical Engineering, Andhra Pradesh, India

³Bluefish Pharmaceuticals Private Limited, Research and Development, Karnataka, India

ABSTRACT

Objectives: Cleaning validation is the procedure used to ensure that the cleaning process has eliminated the residues of drug substance from on the equipment surface after manufacture. A simple, sensitive, robust, and accurate high performance liquid chromatographic method was developed for the quantitative estimation of dipyrindamole in swab samples obtained from the equipment surface after the manufacture of dipyrindamole modified release capsules.

Materials and Methods: The method was developed by using a Hypersil BDS C18 (150×4.6 mm, 5 µm) column with mobile phase containing a mixture of buffer (potassium dihydrogen phosphate buffer, pH 7.0±0.05) and methanol in the ratio of 30:70 v/v. Flow rate was 1.5 mL/min, column temperature was 45°C, and injection volume was 5 µL.

Results: The method was validated and a specificity study was conducted to prove that there was no interference from blank and swab blank at the retention time of dipyrindamole. The limit of detection and limit of quantification (LOQ) were established by using a series of linearity solutions and were found to be 0.041 µg/mL and 0.124 µg/mL, respectively. The method precision at the LOQ level was 8.6% relative standard deviation (RSD), method precision was 0.2% RSD, and ruggedness was 0.3% RSD. The method was accurate from the concentration of 0.13 µg/mL to 21.80 µg/mL and the recovery results met the acceptance criteria. The linearity of the method was found from 0.12 µg/mL to 20.14 µg/mL and the r^2 value was 0.997. The robustness for the flow rate, wavelength, column temperature, buffer pH, and mobile phase ratio variations was tested, and all the system suitability parameters were met.

Conclusion: The method validation was performed as per the regulatory requirements and guidelines. The validation parameters met the acceptance criteria and the proposed method can be applied for the intended routine swab analysis.

Key words: Dipyrindamole, swab, method development, validation, cleaning

ÖZ

Amaç: Temizlik validasyonu, temizleme sürecinin üretimden sonra ilaç maddesinin ekipman yüzeyinden kalıntılarını uzaklaştırdığından emin olmak için kullanılan bir prosedürdür. Dipiridamolün modifiye salım yapan kapsüllerinin üretiminden sonra ekipman yüzeyinden alınan sürüntü örneklerde dipiridamolün kantitatif tahmini için basit, hassas, kararlı ve kesin bir yüksek performanslı sıvı kromatografisi yöntemi geliştirilmiştir.

*Correspondence: E-mail: valavalasriram@gmail.com, Phone: +91 8884426522 ORCID-ID: orcid.org/0000-0001-5923-9241

Received: 03.11.2018, Accepted: 17.01.2019

©Turk J Pharm Sci, Published by Galenos Publishing House.

Gereç ve Yöntemler: Yöntem, hipersil BDS C18 (150×4,6 mm, 5 µm) kolonu kullanılarak hareketli faz içeren tampon (potasyum dihidrojen fosfat tamponu, pH 7,0±0,05) ve metanolün 30:70 (h/h) oranında kullanılmasıyla geliştirilmiştir. Akış hızı 1,5 mL/min, kolon sıcaklığı 45°C ve enjeksiyon hacmi 5 µL olarak belirlenmiştir.

Bulgular: Yöntem valide edilmiştir ve özgünlük çalışması, kör ve sürüntü körünün dipiridamol alkonma zamanı ile girişim göstermediğini kanıtlamak için gerçekleştirilmiştir. Deteksiyon sınırı ve kantifikasyon sınırı bir seri doğrusallık çözeltisi kullanılarak belirlenmiştir ve sırasıyla 0,041 µg/mL ve 0,124 µg/mL olarak bulunmuştur. Yöntemin kesinliği kantifikasyon sınırında %8,6 relatif standart sapma (RSD), yöntem kesinliği %0,2 RSD ve dayanıklılığı %0,3 RSD bulunmuştur. Yöntem 0,13 µg/mL ile 21,80 µg/mL konsantrasyonu aralığında kesin bulunmuştur ve geri kazanım sonuçları kabul edilebilirlik kriterlerini karşılamaktadır. Yöntemin doğrusallığı 0,12 µg/mL ile 20,14 µg/mL arasında bulunmuştur ve bulunan r^2 değeri 0,997'dir. Akış hızı, dalga boyu, kolon sıcaklığı, tampon pH'sı ve hareketli faz oranındaki değişimler için dayanıklılık çalışması yapılmıştır ve tüm sistem uygunluk parametreleri karşılanmıştır.

Sonuç: Yöntem validasyonu, düzenleyici gereklilikler ve kurallara göre gerçekleştirilmiştir. Validasyon parametreleri kabul kriterlerini karşılamıştır ve önerilen bu yöntem amaçlanan sürüntü rutin analizi için kullanılabilir.

Anahtar kelimeler: Dipiridamol, sürüntü, yöntem geliştirme, validasyon, temizleme

INTRODUCTION

Cleaning validation should be performed to confirm the efficiency of any cleaning procedure when pharmaceutical products are in contact with equipment. In the pharmaceutical manufacturing industry it is well known that the manufacturing equipment and manufacturing area should be cleaned after every manufacturing process of drug products and this process is strictly endorsed by the regulatory authorities. Cleaning validation is a vital analytical responsibility of the quality management system in the pharmaceutical industry and this process ensures that the cleaning procedure effectively eliminates the residue from the manufacturing equipment and manufacturing area below a predetermined tolerable limit. The cleaning process ensures the product quality of different products, is a helpful tool to avoid cross-contamination, and is a requirement of European Union guidelines for Good Manufacturing Practice and the United States Food and Drug Administration (USFDA). Cleaning validation involves two different activities: one is development and validation of the cleaning process used to remove the drug from the manufacturing equipment surfaces and the other is development and validation of the methods used to measure the residues on the surfaces of the manufacturing equipment. Evaluation of the sensitivity and specificity of the analytical method used to detect residue is critical. The residue analytical method should be able to detect and quantify the drug substance at a very low level from the manufacturing equipment. The residue analytical procedure should be tested in the mixture of sampling method used to show that residue can be recovered from the equipment surface with the specified levels in the accuracy study before concluding the sampling procedure. In general, two types of sampling procedure were found acceptable by the regulatory authorities and frequently practicing pharmaceutical industries. The popular sampling method is the direct method of sampling on the surface of the manufacturing equipment and another method is to use rinse solutions from the manufacturing equipment. The positive aspect of direct sampling of the equipment surface is that the areas hardest to clean and that are reasonably available can be projected, important for finding a level of residue per given surface area. In the case of rinse samples, the two benefits of using rinse samples are that a larger surface area may be sampled and unreachable systems or ones that cannot be routinely disassembled can be sampled

and estimated. The disadvantage of rinse samples is that the residue may not be soluble or may be physically occluded in the manufacturing equipment surface area.

With direct surface sampling there is a possibility of interference from the swab sticks as they have some glue content and before finalizing the sampling procedure the specificity also should be evaluated. The selection of the extraction solvent is a critical step during the development of the cleaning method, the drug substance should be soluble and recoverable across the accuracy swab sample level, and the results should meet the acceptance criteria.

The drug product manufacturer's rationale for the residue limits established should be logical based on the manufacturer's scientific knowledge of the materials involved. It is important to describe the analytical method sensitivity of the residue method in order to fix sensible acceptable limits. According to the USFDA, the limit should be based on logical criteria, involving the risk associated with residues of determined products. The calculation of an acceptable limit of residues and a maximum allowable carryover for an active pharmaceutical ingredient in the production equipment should be based on therapeutic doses, toxicity, and a general limit (10 µg). Several mathematical formulas have been proposed to establish the acceptable residual limit.¹⁻¹⁷

The drug substance dipiridamole (Figure 1): chemical name: 2,2',2'',2'''-[4,8-di (piperidin-1-yl) pyrimido [5,4-d] pyrimidine-2,6-diyil] dinitrilo] tetraethanol, CAS Registry number: 58-32-2, molecular formula: C₂₄H₄₀N₈O₄, molecular mass: 504.6, appearance: bright yellow, crystalline powder, solubility:

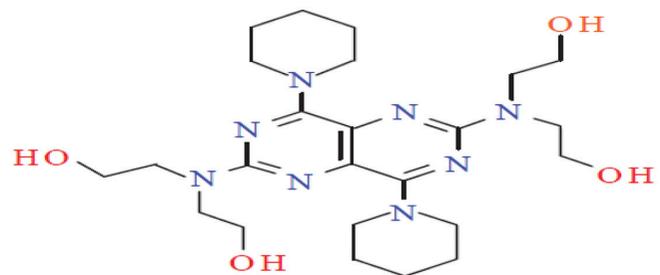


Figure 1. Structure of dipiridamole

practically insoluble in water, slightly soluble in acetone, soluble in anhydrous ethanol, and it dissolves in dilute mineral acids.

The aim of the present study was to develop a simple and fast analytical method for the estimation of the dipyrnidamole content in swab samples after the manufacture of dipyrnidamole modified release capsules on the surface of the manufacturing equipment and to meet the regulatory requirements. Hence, the developed method was subjected to analytical validation with respect to specificity, linearity, precision, accuracy, robustness, and ruggedness. The specificity studies were performed on the diluent, swab, and placebo during the analytical method validation as per International Council for Harmonisation of Technical Requirements for Pharmaceuticals for Human (ICH) guidelines.¹⁸ The developed and validated method can be used for the routine swab samples analysis.

MATERIALS AND METHODS

Chemicals and reagents

High performance liquid chromatographic (HPLC)/analytical grade water, potassium dihydrogen phosphate, methanol, and sodium hydroxide were used. The dipyrnidamole drug substance and dipyrnidamole working standard were supplied by Bluefish Pharmaceuticals Private Limited (India).

Equipment

The analytical method was developed and validated by using the HPLC from Agilent 1200 with a VWD/PDA detector. The output signal was monitored and processed using specific software. An analytical balance from Mettler Toledo, a Sartorius pH meter, and a refrigerator were used.

Chromatographic conditions

The proposed method was developed using a Hypersil BDS C18 (150×4.6 mm) 5 µm column with mobile phase containing a mixture of mobile phase (buffer: potassium dihydrogen phosphate buffer, pH 7.0±0.05) and methanol solution in the ratio of 30:70 v/v. The flow rate was 1.5 mL/min with a column temperature of 45°C, detection wavelength of 295 nm, and sample injection volume of 5 µL.

Preparation of solutions

Diluent solution

Methanol was used as diluent.

Preparation of dipyrnidamole standard solution

Weigh and transfer about 50 mg of dipyrnidamole working standard into a 50 mL volumetric flask. Add about 35 mL of diluent and sonicate for 2 to 3 min until the material is completely dissolved. Pipette out 1 mL of the above solution into a 100 mL volumetric flask, make it up to volume with diluent, and mix well. Pipette out 4 mL of the above solution into a 10 mL volumetric flask, make it up to volume with diluent, and mix well.

Preparation of test tubes and swabs

Take the clean and dry test tubes. Rinse the required number of swabs and test tubes with about 10 mL of swabbing solvent two

times. Squeeze out the swab against the side of the test tubes and discard the swabbing solvent.

Preparation of blank solution

Transfer 10 mL of swabbing solvent to the above cleaned test tube. Place a cleaned swab into the test tube and sonicate for 10 min. Squeeze the swab and take it out and mix well.

Preparation of test solution

Transfer 10 mL of swabbing solvent to the above cleaned test tube. Place a cleaned swab into the test tube to wet the swab with swabbing solvent. Squeeze the swab by pressing it against wall of the test tube. Do the swabbing at the prescribed area of equipment. After swabbing, place the swab in the above test tube containing swabbing solvent and sonicate for 10 min.

Squeeze the swab by pressing it against the wall of the test tube and take it out and filter it through a membrane filter and inject.

System suitability criteria

The present relative standard deviation of the dipyrnidamole peak area for six replicate injections should not be more than 5.0.

The tailing factor for dipyrnidamole peak in standard solution should not be more than 2.0.

The present relative standard deviation of dipyrnidamole peak retention time for six replicate injections should not be more than 1.0.

The % recovery for dipyrnidamole check standard solution should not be less than 95.0% and 105.0%.

RESULTS AND DISCUSSION

Method development

During the method development stage, the standard solution was prepared with a known concentration, blank solution was scanned in a ultraviolet spectrophotometer, and the diluent blank (Figure 2) and dipyrnidamole working standard (Figure 3) spectrums collected to check the wavelength maxima.

The dipyrnidamole peak retention time was about 2.8 min in the chromatogram and the relative standard deviation for the six replicate injections was 0.2% and this proved that the method is reproducible. The accuracy study was conducted by spiking a known concentration of dipyrnidamole solution in an SS plate of 0.4 µg/mL, 4 µg/mL, and 6 µg/mL and the % recovery for all the levels was calculated and the results were found in the range of 99% to 100% and this proved that the method is accurate. The linearity study was conducted by spiking a known concentration of dipyrnidamole solution of about 0.4 µg/mL, 1 µg/mL, 2 µg/mL, 4 µg/mL, 5 µg/mL, and 6 µg/mL, the square of correlation coefficient was calculated and found to be 0.999, and this proved that the method is linear from 0.4 µg/mL to 6 µg/mL. Based on the above-mentioned satisfactory results, the below-mentioned chromatographic conditions were finalized for the quantitative estimation of dipyrnidamole in the swab samples from drug product manufacturing of the dipyrnidamole modified release capsules equipment surface after manufacturing. The

chromatographic conditions are a Hypersil BDS C18 (150×4.6 mm) 5 μ m column with mobile phase containing a mixture of mobile phase (buffer: potassium dihydrogen phosphate buffer, pH 7.0±0.05) and methanol in the ratio of 30:70 v/v. The flow rate was 1.5 mL/min with column temperature of 45°C and detection wavelength of 295 nm. The injection volume was 5 μ L with isocratic flow. Hence, this method can be introduced for routine swab analysis.

Method validation

The proposed analytical method for the quantitative estimation of dipyrnidamole in swab samples from drug product manufacturing of the dipyrnidamole modified release capsules equipment surface area after manufacturing was validated as per the ICH.¹⁸ The validation characteristics specificity, precision, accuracy, linearity, range, ruggedness, and robustness were determined.

System suitability

To check the system suitability criteria, solutions were prepared and injected as per the test method of analysis. All the system suitability parameters were found well within the acceptance criteria. A summary of the system suitability is given in Table 1.

Table 1. System suitability criteria and results

Parameter	Acceptance criteria	Result
The present relative standard deviation of dipyrnidamole peak area for six replicate injections	Not more than 5.0	2.0%
The tailing factor for dipyrnidamole peak in standard solution	Not more than 2.0	1.2
The present relative standard deviation of dipyrnidamole peak retention time for six replicate injections	Not more than 1.0	0.2%
The % recovery for dipyrnidamole check standard solution	Not less than 95.0 and not more than 105.0	96.7%

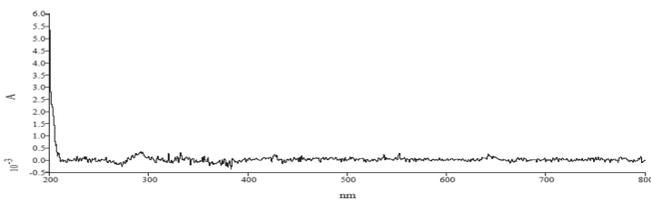


Figure 2. Spectrum of diluent blank

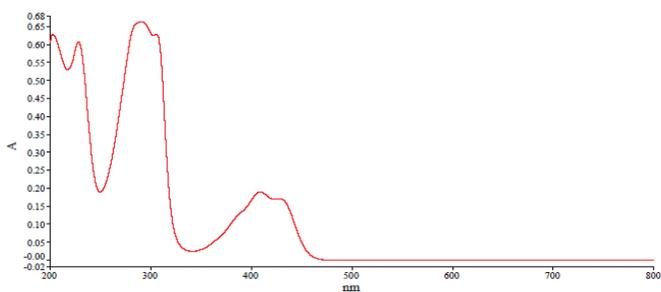


Figure 3. Spectrum of standard

Specificity

To study the specificity, required solutions like diluent as blank, swab blank, and standard solution were prepared and injected as per the test method. It was observed that there was no peak interference at the retention time of dipyrnidamole from blank and swab blank solutions in the chromatogram. Specimen chromatograms of diluent as blank are shown in Figure 4, swab blank in Figure 5, and standard in Figure 6, and overlaid chromatograms of diluent as blank, swab blank, and standard in Figure 7.

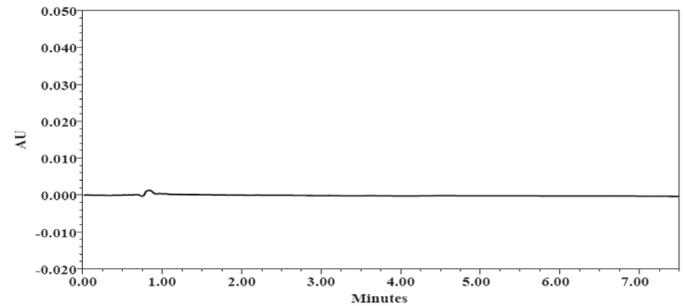


Figure 4. Specimen diluent blank chromatograms

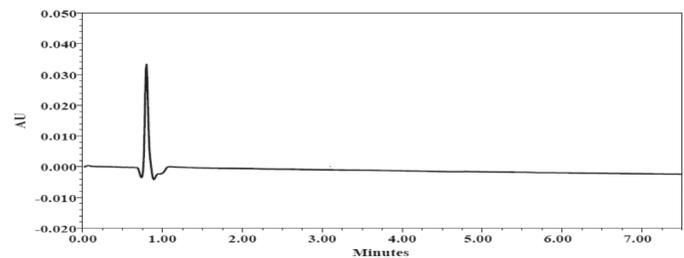


Figure 5. Specimen swab blank chromatograms

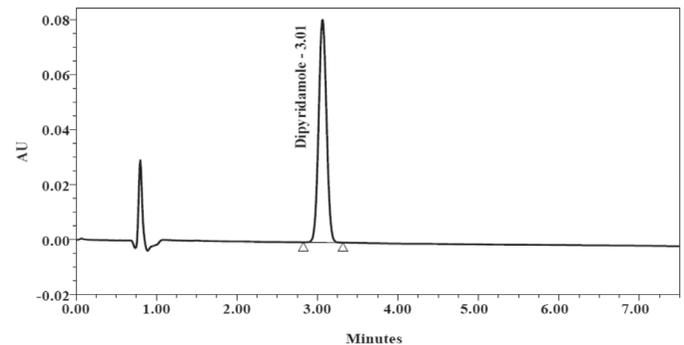


Figure 6. Specimen standard chromatograms

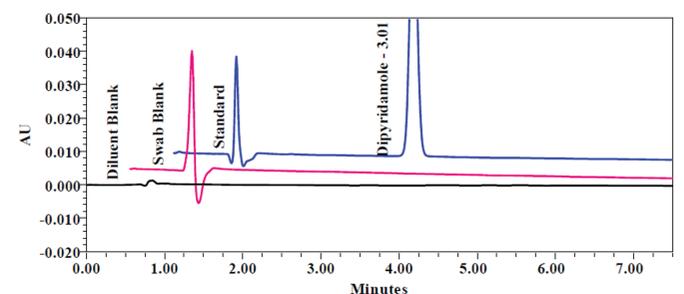


Figure 7. Specimen overlaid chromatograms

Estimation of limit of detection (LOD) and limit of quantification (LOQ)

To evaluate the concentration limits as LOD and LOQ, a series of linearity solutions were prepared ranging in concentration from about 0.1 µg/mL to 2.0 µg/mL and the square of correlation coefficient, slope of the curve, and y-intercept were determined. The LOQ was calculated based on the standard deviation of the response and the slope as mentioned in the formula below. A summary of the results of the LOD and LOQ estimation study is given in Table 2 and Figure 8.

$$LOQ = \frac{10 \times \sigma}{S}$$

where

- σ = the standard deviation of the response
- S = the slope of the calibration curve

Method precision at LOQ level

The method precision at LOQ concentration was determined by preparing six replicate test preparations (n=6) of dipyridamole stock solution and samples were analyzed as per the test method. The % relative standard deviation (RSD) for response of dipyridamole six replicate injections was calculated and found within the acceptance criteria. A summary of the method precision for the LOQ level study results is given in Figure 9.

Method precision (repeatability)

Precision was determined by preparing six replicate test preparations (n=6) of dipyridamole stock solution spiked onto an SS plate (4x4 inch) and samples were analyzed as per the test method. The % recovery for replicate injections and % RSD for response of six replicate injections of dipyridamole were calculated and found within the acceptance criteria. A summary of the method precision study results is given in Figure 10.

Table 2. Estimation of LOD and LOQ

Description	Dipyridamole
Square of correlation coefficient (r ²)	0.999
Slope	11073.25
Y-intercept	50.4388
Limit of detection (µg/mL)	0.041
Limit of quantification (µg/mL)	0.124

LOD: Limit of detection, LOQ: Limit of quantification

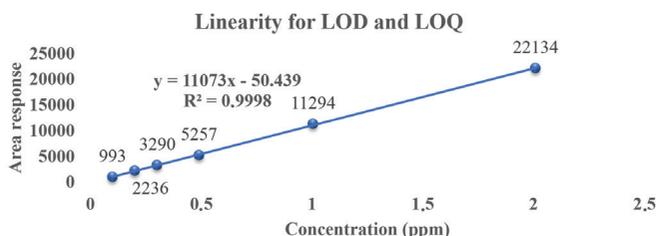


Figure 8. Linearity for LOD and LOQ

LOD: Limit of detection, LOQ: Limit of quantification

Accuracy

In the accuracy study, a series of sample solutions were prepared in triplicate six preparations for lower level (LOQ) and higher level (500%) by spiking the dipyridamole drug substance stock onto an SS plate (4x4 inch) at LOQ 50%, 100%, 200%, 300%, and 500% and analyzed as per the test method. The spiked concentrations of dipyridamole were 0.12 µg/mL, 2.01 µg/mL, 4.03 µg/mL, 8.05 µg/mL, 12.08 µg/mL, and 21.14 µg/mL. Individual % recovery, mean % recovery, % RSD, and squared correlation coefficient for linearity of the test method were calculated and the results were found within the predefined acceptance criteria. A summary of the accuracy study results is given in Table 3 and Figure 11.

Linearity

The linearity was studied by analyzing the standard solutions. A series of solutions of dipyridamole standard solutions were prepared in the range of LOQ to about 500% and injected into the HPLC system. Linearity of detector response was established by plotting a graph of concentration vs. response of dipyridamole. The detector response was found to be linear from about LOQ to 500% and injected into the HPLC system and analyzed as per the test method. The concentrations of

Table 3. Accuracy data of dipyridamole

Spike level	% Mean recovery of dipyridamole	Average amount added (µg/mL)	Average amount found (µg/mL)
Level-1	101.5	0.12	0.13
Level-2	97.5	2.01	1.97
Level-3	98.7	4.03	3.98
Level-4	99.7	8.05	8.03
Level-5	105.1	12.08	12.70
Level-6	103.1	21.14	21.80

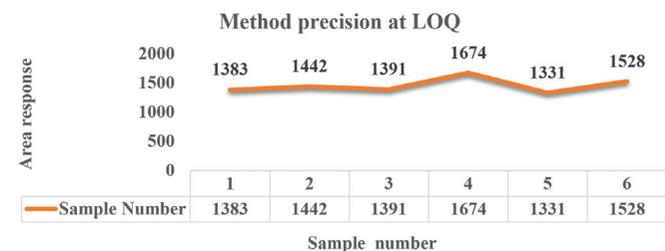


Figure 9. Method precision at LOQ level

LOQ: Limit of quantification

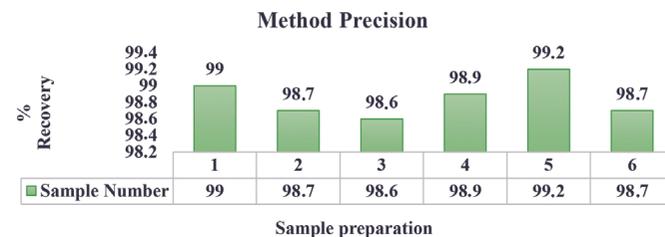


Figure 10. Method precision

dipyridamole were 0.1208 $\mu\text{g/mL}$, 2.0137 $\mu\text{g/mL}$, 4.0274 $\mu\text{g/mL}$, 8.0548 $\mu\text{g/mL}$, 12.0821 $\mu\text{g/mL}$, and 20.1369 $\mu\text{g/mL}$.

The square of correlation coefficient, slope, and % y-intercept at 100% level, and intercept and residual sum of squares were calculated and the results met the acceptance criteria. A summary of the linearity study results is given in Table 4 and Figure 12.

Ruggedness

The intermediate precision was determined by preparing six replicate test preparations (n=6) of dipyridamole stock solution spiked onto an SS plate (4x4 inch) and samples were analyzed as per the test method using a different HPLC system and a different column of the same make by a different analyst on a different day. The % recovery for replicate injections and % RSD for response of six replicate dipyridamole injections were

calculated and met the acceptance criteria. A summary of the ruggedness study results is given in Table 5 and Figure 13.

Solution stability and mobile phase stability

The solution stability of dipyridamole was determined by keeping swab sample solution and standard solutions in tightly capped volumetric flasks at room temperature for 1 day and 2 days and measuring against freshly prepared standard solution. The standard solution and swab sample solutions was found stable for 2 days at room temperature.

The stability of the mobile phase was also determined by freshly prepared solutions of dipyridamole at 1 day and 2 days. The mobile phase was found stable for 2 days at room temperature.

Robustness

Robustness of the proposed method was performed by keeping the chromatographic conditions constant with the following deliberate variations:

- Change in flow rate
- Change in wavelength
- Change in mobile phase buffer pH
- Change in HPLC column temperature
- Change in mobile phase composition

The standard solution was injected in replicate for each above mentioned change. The system suitability parameters were recorded for dipyridamole peak and the system suitability

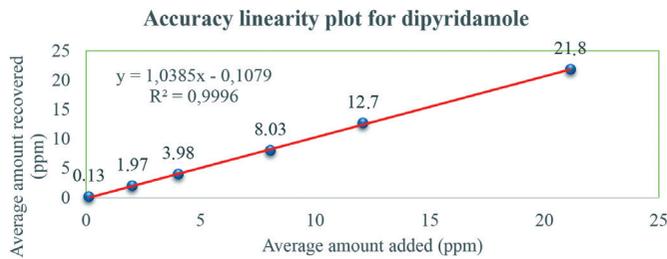


Figure 11. Accuracy linearity plot for dipyridamole

Table 4. Linearity data of dipyridamole

Linearity level	% Linearity	Concentration ($\mu\text{g/mL}$)	Area response
Level-1	LOQ	0.1208	1514
Level-2	50%	2.0137	24558
Level-3	100%	4.0274	49035
Level-4	200%	8.0548	97506
Level-5	300%	12.0821	152086
Level-6	500%	20.1369	231128
Square of correlation coefficient (r^2)			0.997
Slope			11622.7
Y-intercept			2686.68
Residual sum of squares			122556978.290215

LOQ: Limit of quantification

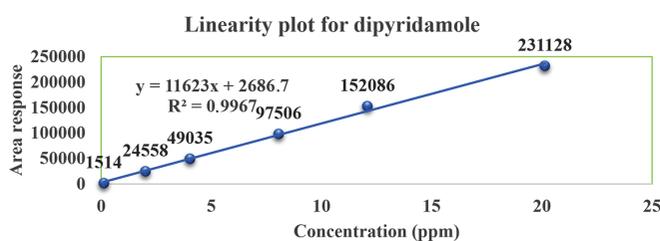


Figure 12. Linearity plot for dipyridamole

Table 5. Ruggedness data

Sample no.	Method precision % recovery	Intermediate precision % recovery
1	99.0	102.6
2	98.7	103.0
3	98.6	102.5
4	98.9	102.3
5	99.2	102.8
6	98.7	102.3
Mean	98.9	102.6
% RSD	0.2	0.3
Overall % RSD	0.3	

RSD: Relative standard deviation

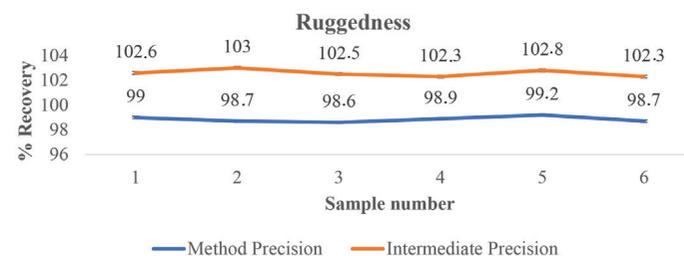


Figure 13. Ruggedness

Table 6. Robustness data

Parameter variation	The present relative standard deviation of dipyrindamole peak area for six replicate injections should not be more than 5.0	The tailing factor for dipyrindamole peak in standard solution should not be more than 2.0	The present relative standard deviation of dipyrindamole peak retention time for six replicate injections should not be more than 1.0	The % recovery for dipyrindamole check standard solution should not be less than 95.0% and 105.0%
Flow 1.30 mL/min	0.3	1.2	0.1	98.0
Flow 1.70 mL/min	0.2	1.2	0.2	98.0
Wavelength 293 nm	0.2	1.2	0.2	97.4
Wavelength 297 nm	0.3	1.2	0.2	97.1
Column temp 40°C	0.2	1.2	0.0	99.5
Column temp 50°C	0.2	1.2	0.0	99.4
Buffer pH 6.8	0.3	1.2	0.0	97.1
Buffer pH 7.2	0.7	1.2	0.3	96.5
Mobile phase ratio 35:65% v/v	0.2	1.2	0.0	99.9
Mobile phase ratio 20:80% v/v	0.2	1.2	0.0	99.7

found well within the acceptance criteria. A summary of the robustness study results is given in Table 6.

The authors declare that no experiments were conducted using human subjects and no ethics committee approval is required for this publication.

APPLICATION OF THE PROPOSED METHOD

The developed analytical method can be applied for the analysis of swab samples from the dipyrindamole drug product manufacturing unit. All the analytical validation parameters met the predefined acceptance criteria and the method was proven to be suitable for analysis of swab samples from drug product manufacturing of the dipyrindamole modified release capsules equipment surface area after manufacturing.

CONCLUSIONS

The developed method was validated as per the ICH guidelines and can be used for the quantitative estimation of dipyrindamole in swab samples from drug product manufacturing of the dipyrindamole modified release capsules equipment surface area after manufacturing. The method was precise, accurate, linear, robust, rugged, and specific and there was no interference found during the specificity study at the retention time of dipyrindamole peak. The validated method can be applied for swab samples from drug product manufacturing of the dipyrindamole modified release capsules equipment surface area after manufacturing.

ACKNOWLEDGMENTS

The authors wish to thank the management of Bluefish Pharmaceuticals Private Limited for their support and encouragement.

Conflicts of interest: No conflict of interest was declared by the authors. The authors alone are responsible for the content and writing of the paper.

REFERENCES

1. EU Guidelines for good manufacturing practice for medicinal products for human and veterinary use, Eudra Lex-Vol. 4. Annex 15: Qualification and Validation, Brussels; 2014.
2. Guide to inspections validation of cleaning processes, US. Food and Drug Administration, Office of Regulatory Affairs, Washington, DC; 1993.
3. Guidance on aspects of cleaning validation in active pharmaceutical ingredient plants, Active Pharmaceutical Committee (APIC); 1999.
4. LeBlance DA. Establishing scientifically justified acceptance criteria for cleaning validation of finished drug products. *Pharm Technol.* 1998;22:136-148.
5. Fourman GL, Mullen MV. Determining cleaning validation acceptance limits for Pharmaceutical manufacturing operations. *Pharm Technol.* 1993;17:54-60.
6. Klinkenberg R, Streef B, Ceccato A. Development and validation of a liquid chromatographic method for the determination of the amlodipine residues on manufacturing equipment surfaces. *J Pharm Biomed Anal.* 2003;32:345-352.
7. Dubey N, Mandhanya M, Jain DK. Cleaning level acceptance criteria and HPLC-DAD method validation for the determination of Nabumetone residues on manufacturing equipment using swab sampling. *J Pharm Anal.* 2012;2:478-483.
8. Ermer J, Miller JH. Method validation in pharmaceutical analysis. Weinheim: WILEY-VCH Verlag GmbH & Co. KGa A; 2005.
9. Eurachem Guide. 2nd ed. The fitness for purpose of analytical methods-A laboratory guide to method validation and related topics; 2014.
10. Kumar VS, Sanjeev T. Overview of cleaning validation in pharmaceutical manufacturing unit. *IJARPB.* 2012;1:154-164.
11. McCormick PY, Cullen LF. Cleaning validation. In: Berry IR, Nash RA, editors. 2nd ed. New York: Marcel Dekker; 1993. p. 319-49.

12. Chudzik GM. General guide to recovery studies using swab sampling methods for cleaning validation. *J Validation Technol.* 1998;5:77-81.
13. Schifflet MJ, Shapiro M. Development of analytical methods to accurately and precisely determine residual active pharmaceutical ingredients and cleaning agents on pharmaceutical surfaces. *Am Pharm Rev Winter.* 2002;4:35-39.
14. Boca B, Apostolides Z, Pretorius E. A validated HPLC method for determining residues of a dual active ingredient anti-malarial drug on manufacturing equipment surfaces. *J Pharm Biomed Anal.* 2005;37:461-468.
15. Forsyth RJ, Haynes DV. Cleaning validation in pharmaceutical research facility. *Pharm Technol.* 1998;22:104-112.
16. Sunil Kumar YV, Mallu UR, Ivaturi KV. RP-HPLC method development and cleaning method validation for the analysis of triclabendazole in veterinary pharmaceutical dosage forms. *International Journal of Chem Tech Research.* 2016;9:316-323.
17. Sunil Kumar Yelamanchi V, Useni Reddy Mallu, Kasi Viswanath Iv, Maheshwara Reddy L. Method Development And Validation Of Cleaning Procedure For Fenbendazole Residual Determination in manufacturing. *Asian J Pharm Clin Res.* 2016;9:507-520.
18. ICH Q2 (R1), "Validation of analytical procedures: text and methodology", Harmonised Tripartite Guideline, in Proceedings of the International Conference on Harmonisation of Technical Requirements for Registration of Pharmaceuticals for Human Use, Chicago, USA, 2005.